

Trace Sulfur determination in metals by the Thermo Scientific FLASH 2000 Elemental Analyzer coupled with FPD detector

Dr. Liliana Krotz, OEA Product Specialist, and Dr. Guido Giazzi, OEA Product Manager, Thermo Fisher Scientific, Milan, Italy.

Key Words

Trace sulfur analysis, sensitivity, accuracy, easier sample handling, automated analysis, assured stability, difficult to destroy

Goal

This application note demonstrates a method for the precise, sensitive and selective determination of low sulfur traces in metals using organic elemental analysis and flame photometric detector.

Introduction

In metallurgy, some elements are of great importance; nitrogen, carbon and sulfur are particularly so where steels are concerned. The addition of nitrogen and carbon improves the properties of the specific metal, although there are certain areas where their presence is undesirable and should be avoided if possible. Sulfur plays an important role in the mechanical properties of steel and alloys, where it is usually present within the range of 10 – 3000 ppm.

Automatic analyzers using dynamic flash combustion have been used for many years for total sulfur determination, but have been limited in many applications due to the detection limit. This limit has been sufficient for most analytical needs up until now, but today, trace sulfur analysis is becoming more demanding.

Trace total sulfur content can be accurately determined by using the Thermo Scientific FLASH 2000 analyzer coupled with a Flame Photometric Detector (FPD) (Figure 1). This method combines the advantages of the elemental analyzer with the sensitivity, selectivity and robustness of a FPD. The coupling is simple and allows total sulfur determination at high and low concentrations (5 – 10 ppm) in the same instrument without matrix effect.

Methods

The elemental analyzer operates according to the dynamic flash combustion of the sample. Samples are weighed in a tin capsule and introduced into the combustion reactor via the Thermo Scientific MAS 200R autosampler together with a proper amount of oxygen. After combustion



Figure 1. FLASH 2000 elemental analyzer coupled with Flame Photometric detector (FPD)

the resultant gases are carried by a helium flow to a layer filled with copper, then to a trap filled with Anhydrone and swept through a GC column that separates the combustion gases; finally being detected by the Flame Photometric detector (FPD) (Figure 2). Total run time is 5-6 minutes. A complete report is automatically generated by the Thermo Scientific Eager Xperience dedicated data handling software and displayed at the end of the analysis.

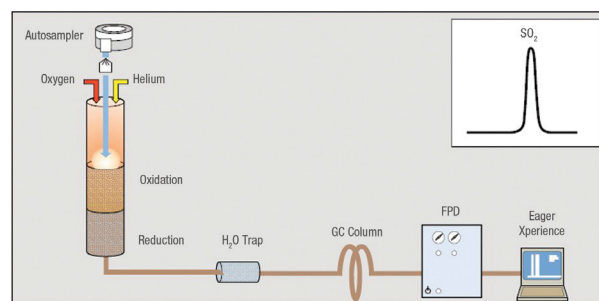


Figure 2. Layout of sulfur determination by FPD detector

Results

Different samples were chosen to demonstrate the performance of the system analyzing different matrices and to show the reproducibility obtained within the system in a large range of trace sulfur content. Metal material - weight sample range 0.5 / 5mg - were cut into small pieces and analyzed without any pre-treatment.

Table 1 shows a typical sequence of analysis. Instrument calibration was performed with cast iron BCR* (0.1670% S) using Quadratic Fit as the calibration method (runs 3 to 6). Figure 3 shows the relative calibration curve obtained. The accuracy of the system was verified by analyzing the same cast iron sample ten times as unknown (runs 7 to 16) as shown in Table 2.

* BCR: Bureau Communautaire de Référence - Community Bureau of Reference

Table 1. Typical sequence

Run	Sample	Type	Weight (mg)
1	Cast Iron BCR	Bypass	
2	Cast Iron BCR	Bypass	
3	Cast Iron BCR	Standard	0.652
4	Cast Iron BCR	Standard	1.090
5	Cast Iron BCR	Standard	1.621
6	Cast Iron BCR	Standard	2.207
7	Cast Iron BCR	Unknown	1.445
8	Cast Iron BCR	Unknown	1.602
9	Cast Iron BCR	Unknown	1.291
10	Cast Iron BCR	Unknown	2.105
11	Cast Iron BCR	Unknown	1.165
12	Cast Iron BCR	Unknown	1.011
13	Cast Iron BCR	Unknown	1.827
14	Cast Iron BCR	Unknown	1.509
15	Cast Iron BCR	Unknown	1.658
16	Cast Iron BCR	Unknown	2.198

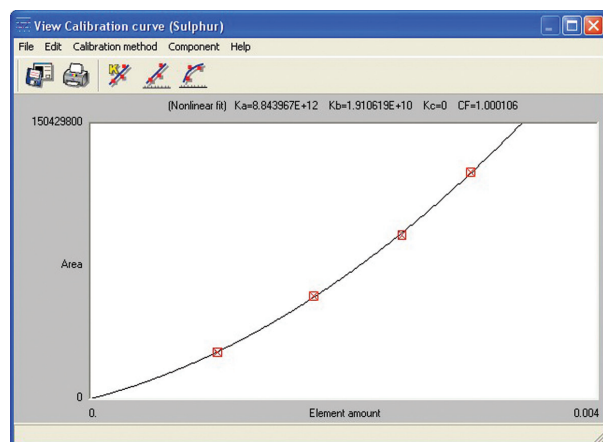


Figure 3. Typical curve calibration

www.thermoscientific.com

©2012 Thermo Fisher Scientific Inc. All rights reserved. ISO is a trademark of the International Standards Organization. All other trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries. This information is presented as an example of the capabilities of Thermo Fisher Scientific Inc. products. It is not intended to encourage use of these products in any manner that might infringe the intellectual property rights of others. Specifications, terms and pricing are subject to change. Not all products are available in all countries. Please consult your local sales representative for details.

Africa-Other +27 11 570 1840
Australia +61 3 9757 4300
Austria +43 1 333 50 34 0
Belgium +32 53 73 42 41
Canada +1 800 530 8447
China +86 10 8419 3588
Denmark +45 70 23 62 60

Europe-Other +43 1 333 50 34 0
Finland/Norway/Sweden
+46 8 556 468 00
France +33 1 60 92 48 00
Germany +49 6103 408 1014
India +91 22 6742 9434
Italy +39 02 950 591

Japan +81 45 453 9100
Latin America +1 561 688 8700
Middle East +43 1 333 50 34 0
Netherlands +31 76 579 55 55
New Zealand +64 9 980 6700
Russia/CIS +43 1 333 50 34 0
South Africa +27 11 570 1840

Spain +34 914 845 965
Switzerland +41 61 716 77 00
UK +44 1442 233555
USA +1 800 532 4752

COMPANY WITH QUALITY MANAGEMENT
SYSTEM CERTIFIED BY DNV
= ISO 9001:2008 =
Thermo Fisher Scientific S.p.A. Milan, Italy is ISO Certified.

AN42185_E 10/12C

Table 2. Test of accuracy

Cast Iron	%S	Average %S	RSD%
Run 7	0.1645		
Run 8	0.1642		
Run 9	0.1696		
Run 10	0.1703		
Run 11	0.1637	0.1675	1.8158
Run 12	0.1726		
Run 13	0.1653		
Run 14	0.1695		
Run 15	0.1685		
Run 16	0.1666		

Table 3 shows sulfur determination in various metal and alloy samples analyzed several times. All data were obtained with a good reproducibility and no matrix effect was observed when changing sample nature.

Table 3. Reproducibility of sulfur determination.

Sample	S ppm	Average S ppm	RDS %
Carbon steel	242	242.5	0.29
	243		
Bronze	158	157	2.60
	153		
	160		
	153		
Steel 1	162	199	3.66
	205		
	193		
	204		
	190		
Steel 2	205	53	2.45
	52		
	54		
	52		
	55		
CrMoNi alloy	53	68	4.21
	72		
	71		
	67		
	66		

Conclusion

The Thermo Scientific FLASH 2000 elemental analyzer coupled with a FPD detector is the ideal solution for the analysis of trace concentration of sulfur in metals in terms of stability, accuracy, reproducibility, sensitivity and automation without matrix effect.

Thermo
SCIENTIFIC
Part of Thermo Fisher Scientific